

1/13

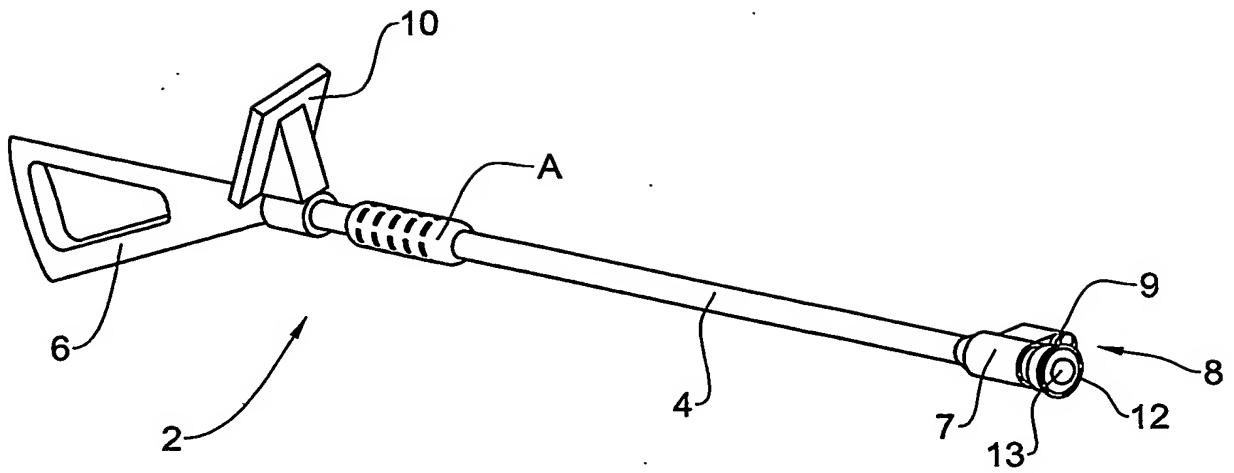


FIG. 1

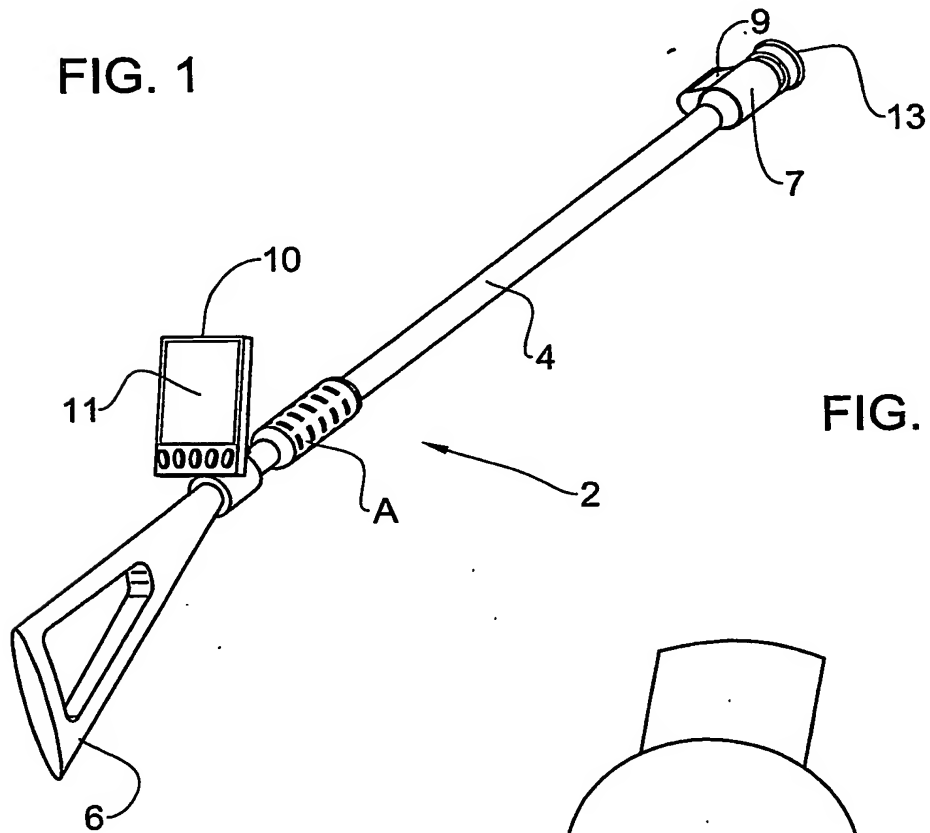


FIG. 2

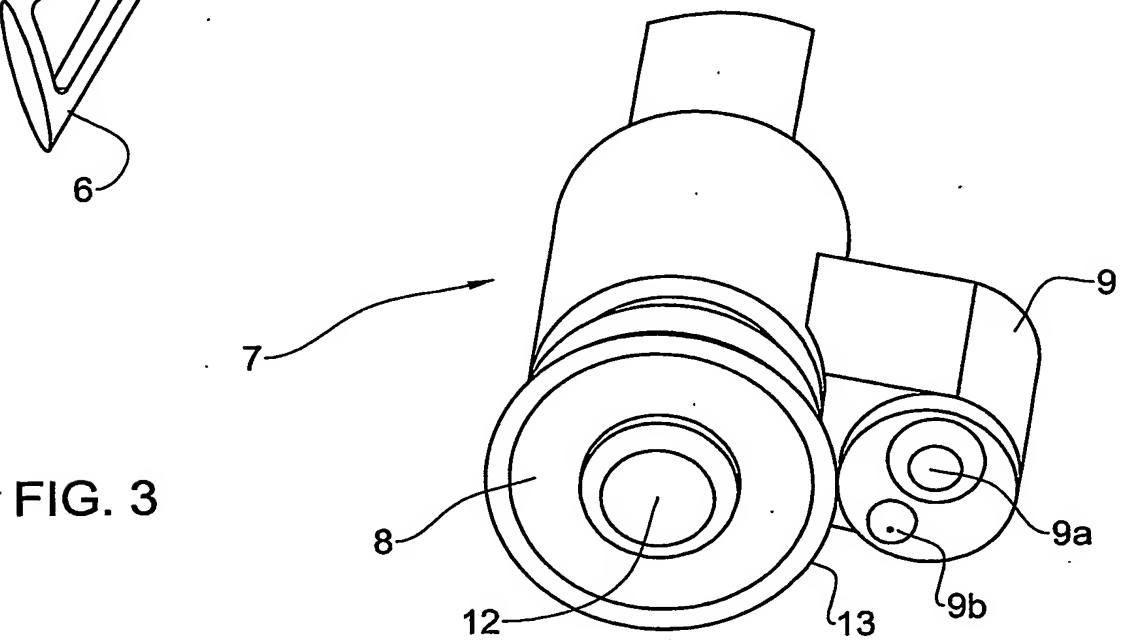


FIG. 3



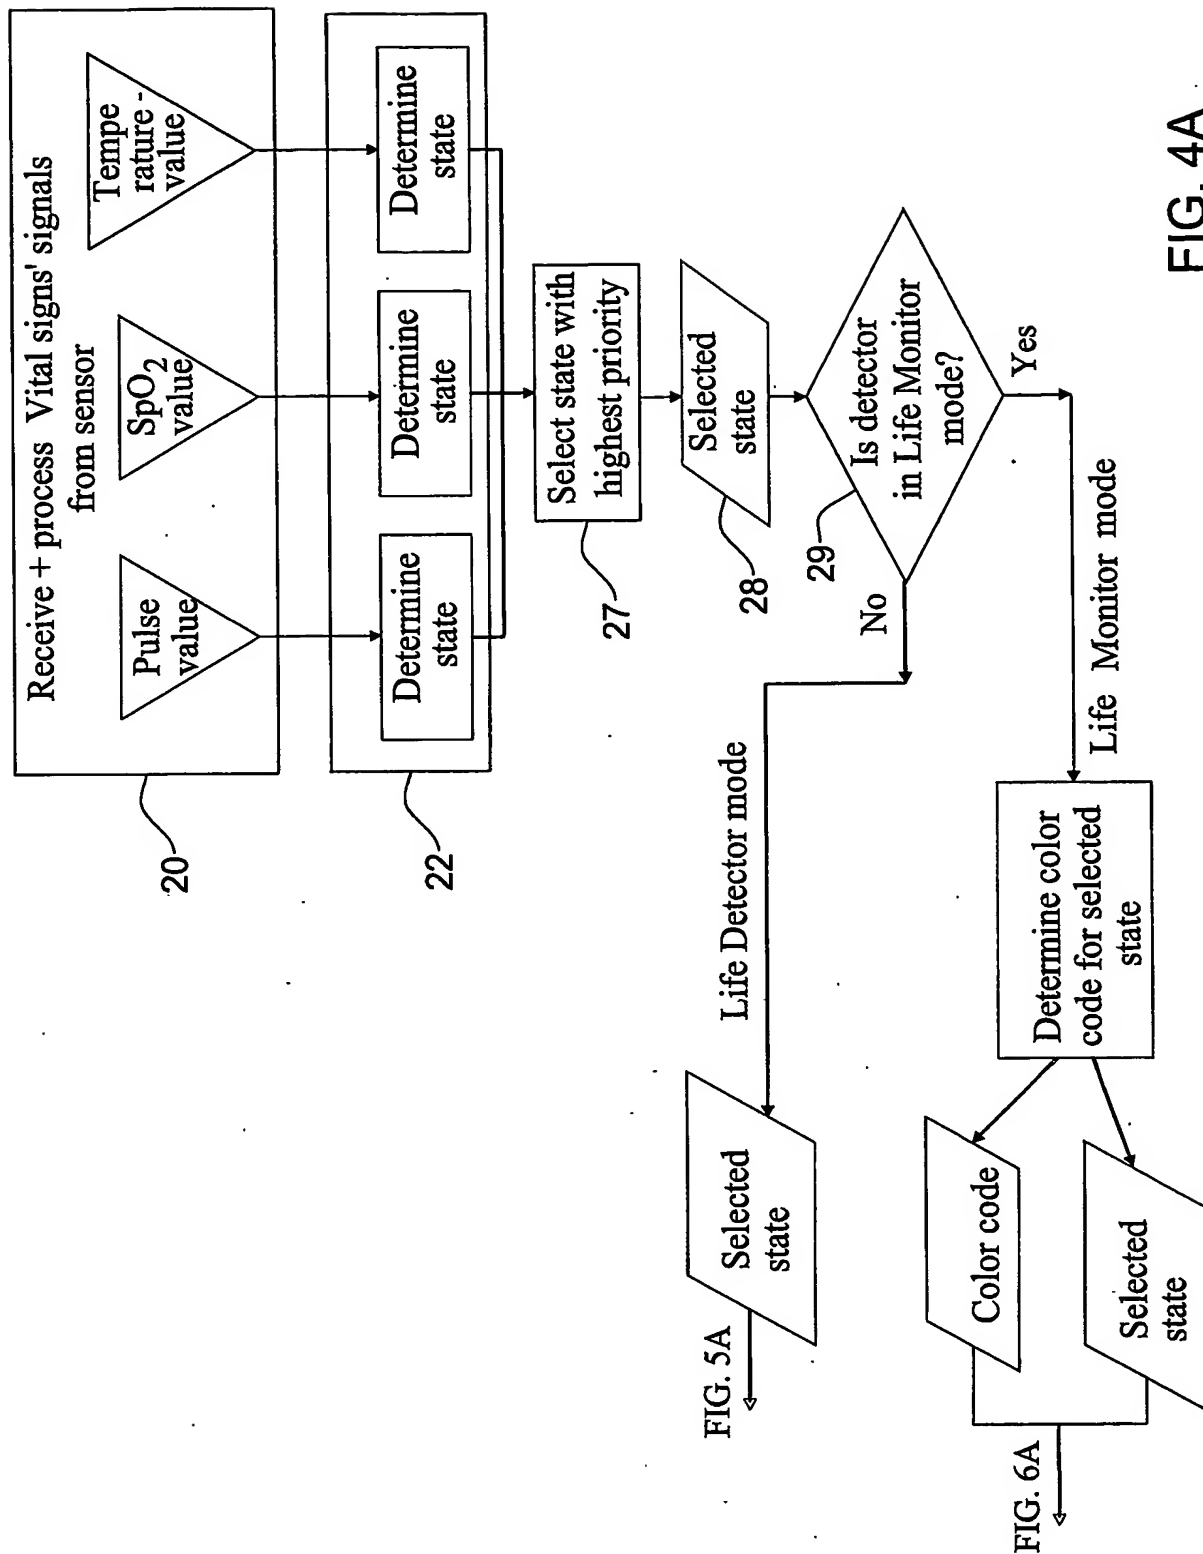


FIG. 4A

3/13

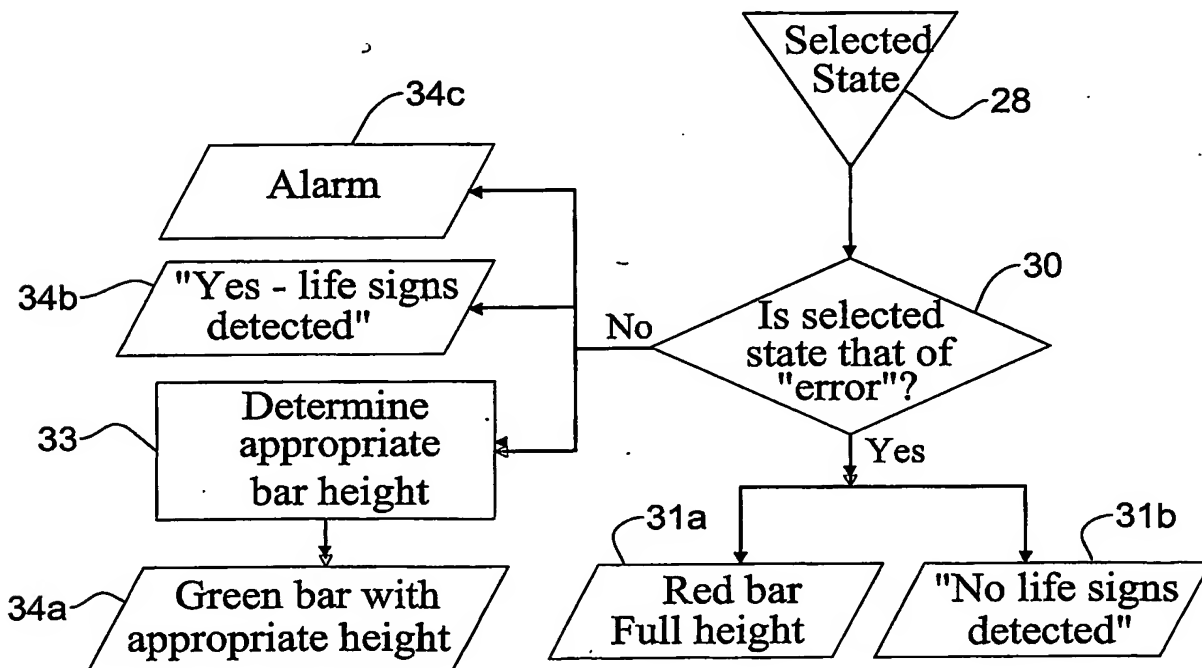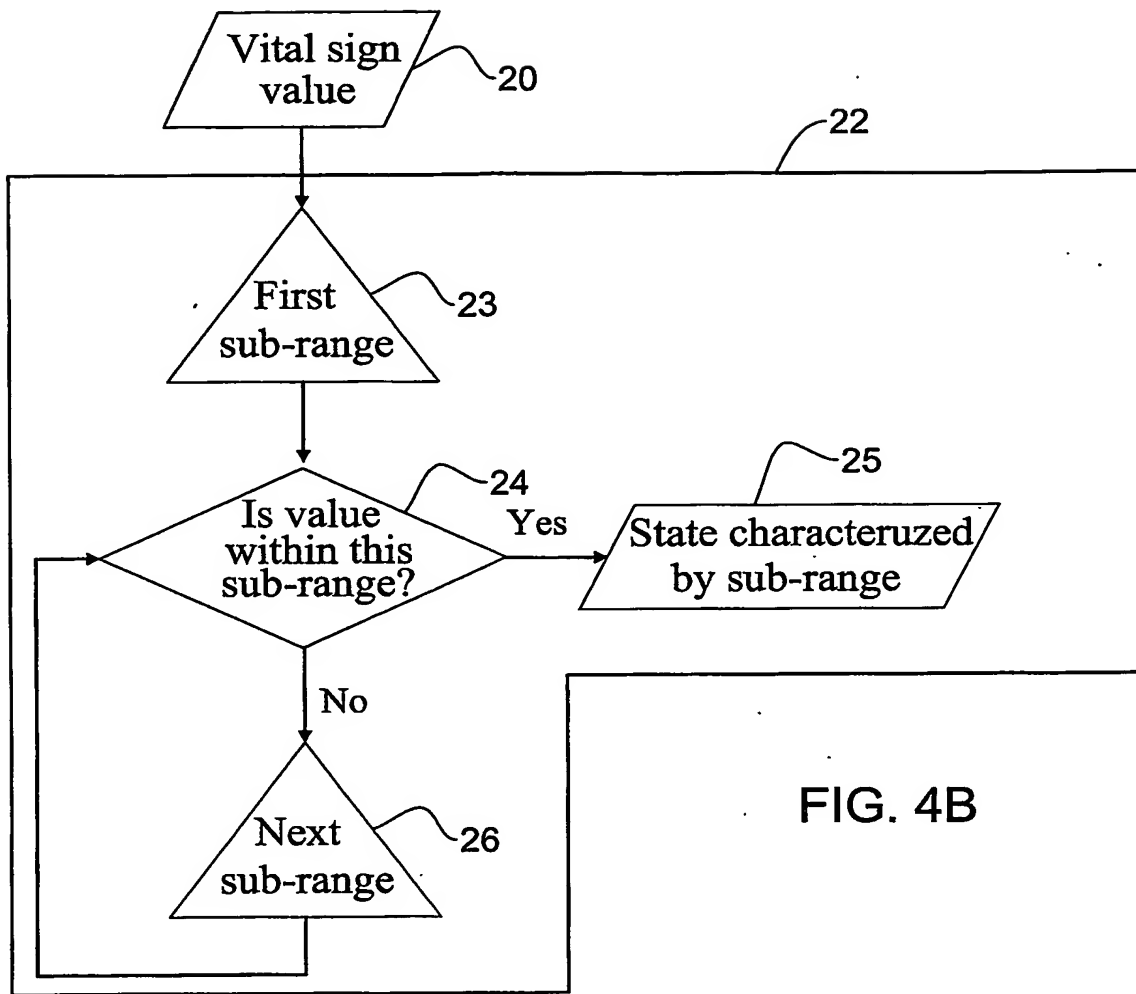

4/13

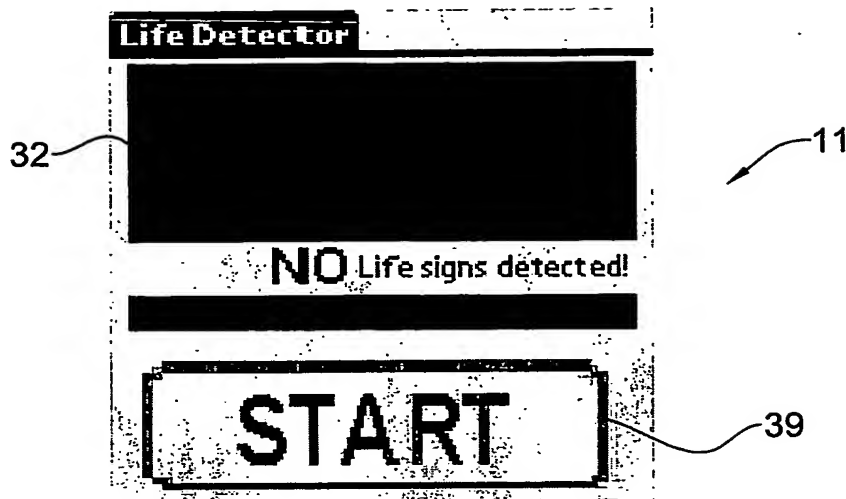


FIG. 5B

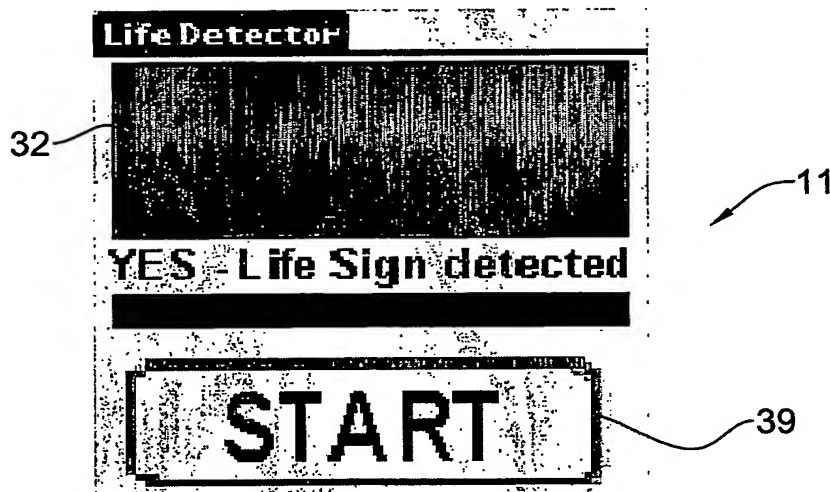


FIG. 5C

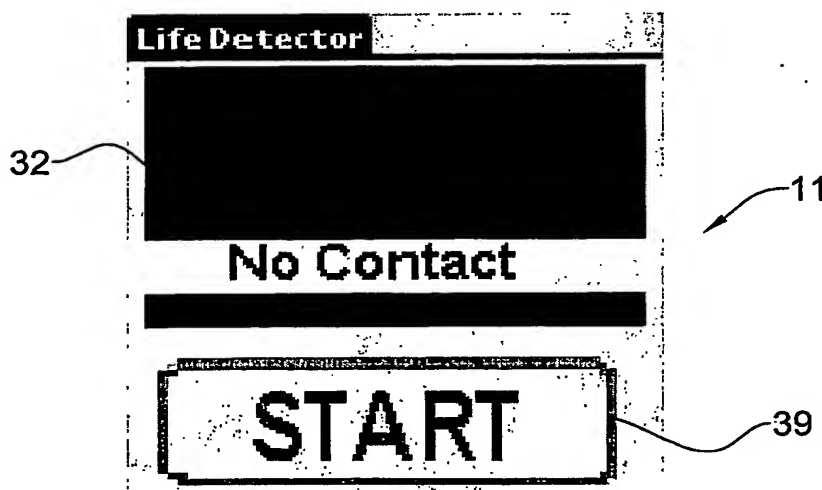


FIG. 5D

5/13

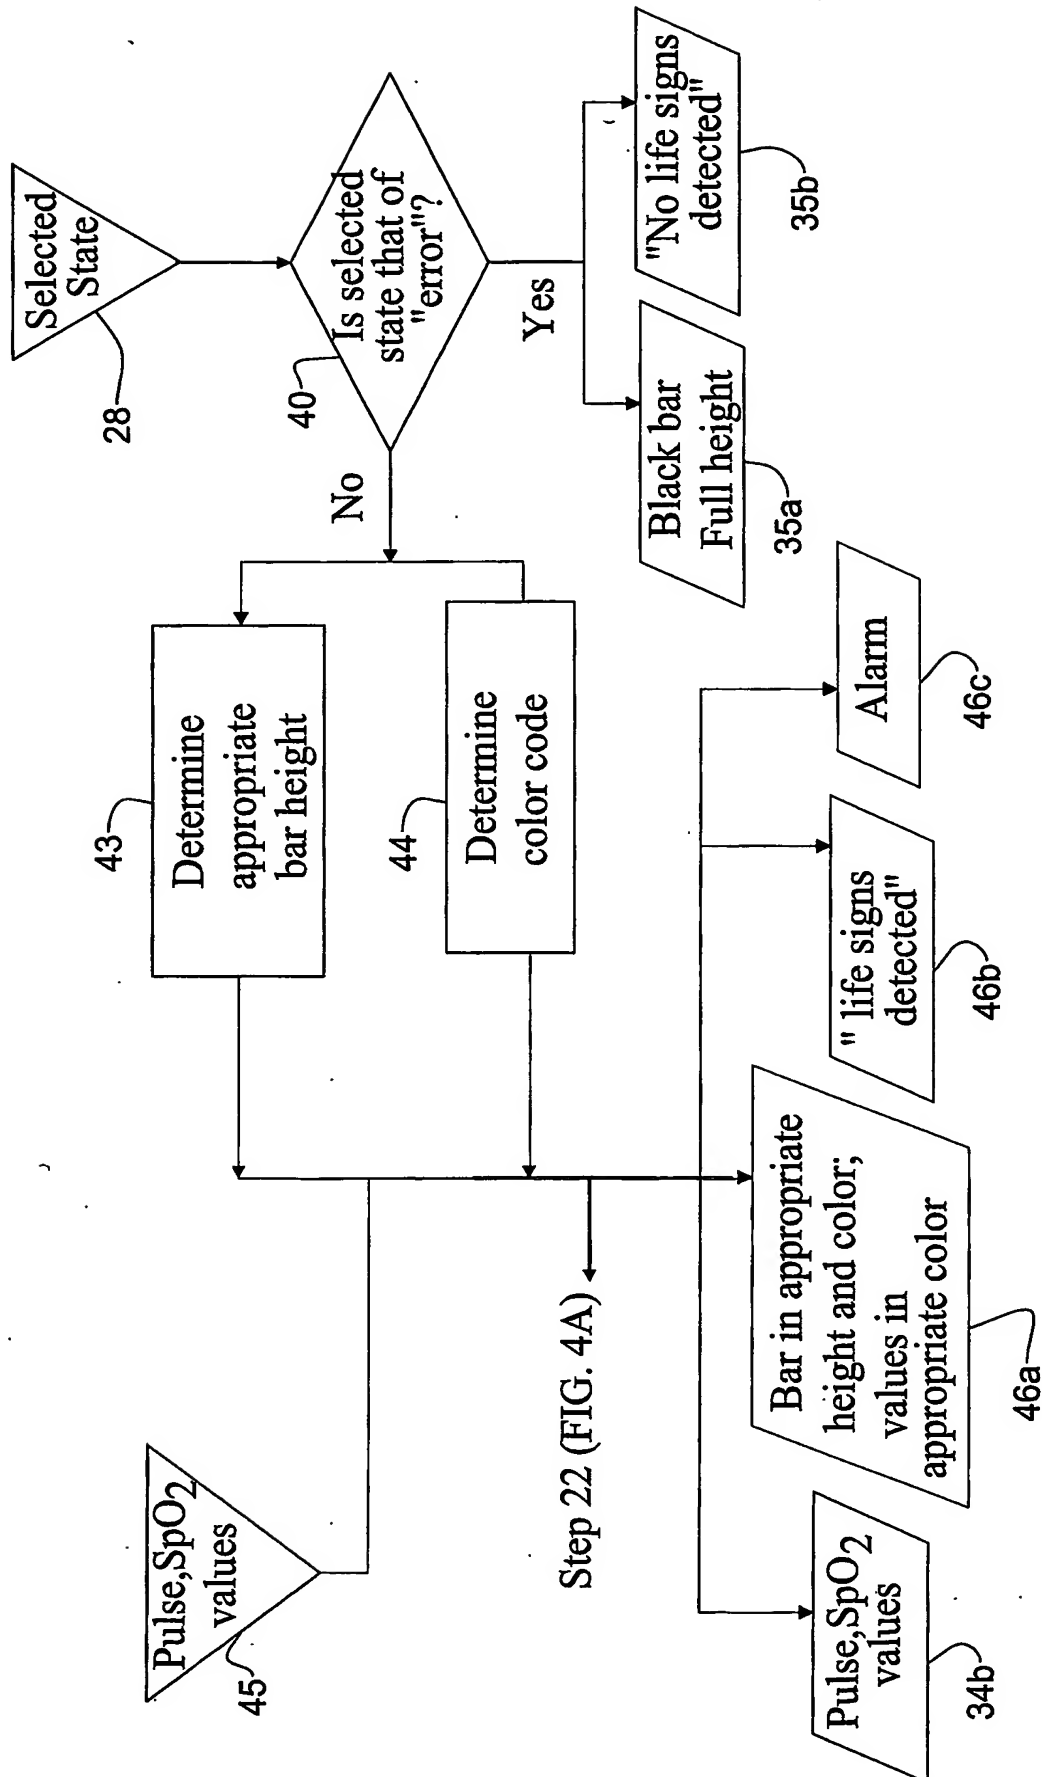


FIG. 6A

6/13

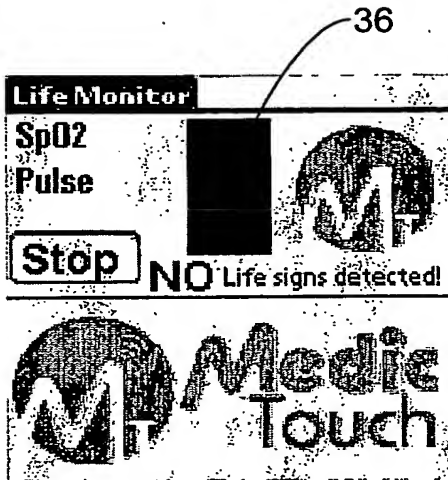


FIG. 6B

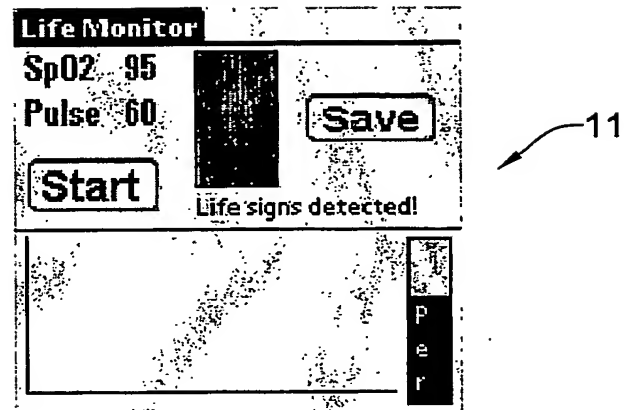


FIG. 6C

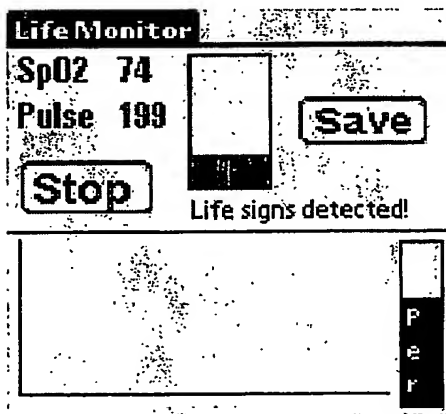


FIG. 6D

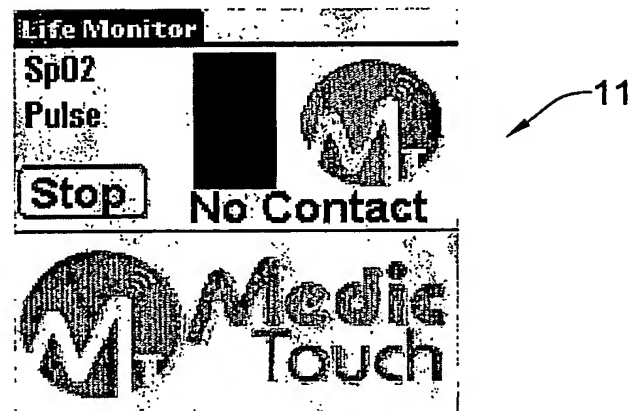


FIG. 6E

7/13



FIG. 8A

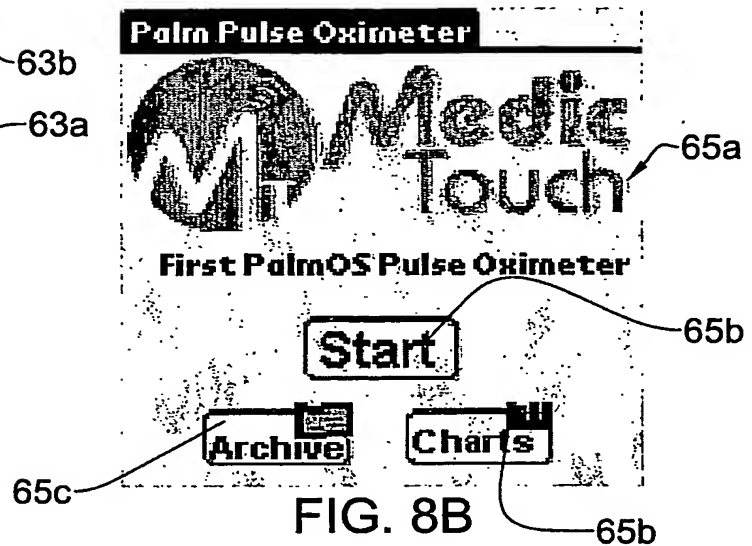


FIG. 8B

Counters	
No vital signs detected	267
High-Risk condition	4
Risk condition	22
Moderate condition	14
Normal condition	35
Total number checked	342
<input type="button" value="Done"/> <input type="button" value="Cancel"/> <input type="button" value="Reset"/> <input type="button" value="Send"/>	

FIG. 8C

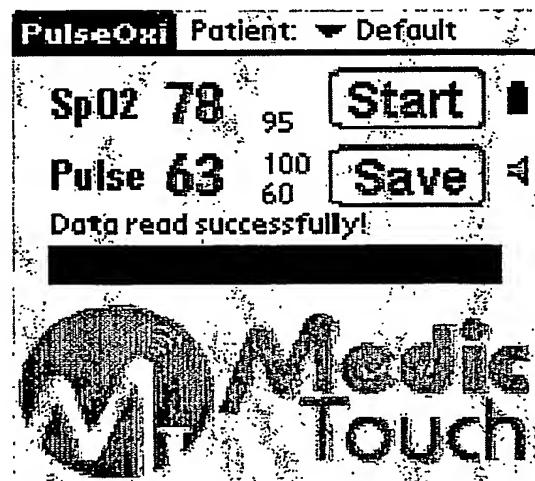


FIG. 8D

Measurements		▼ Default	
Date	O2	Pulse	Notes
5/1/02 7:51	97	102	S
5/1/02 7:51	95	70	S
5/1/02 7:51	96	66	S
5/1/02 7:51	97	82	S
<input type="button" value="Done"/> <input type="button" value="New"/> <input type="button" value="Edit"/> <input type="button" value="Clear"/>			

FIG. 8E

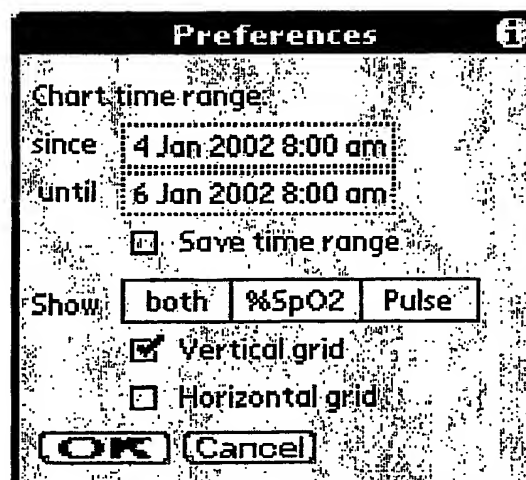


FIG. 8F

8/13

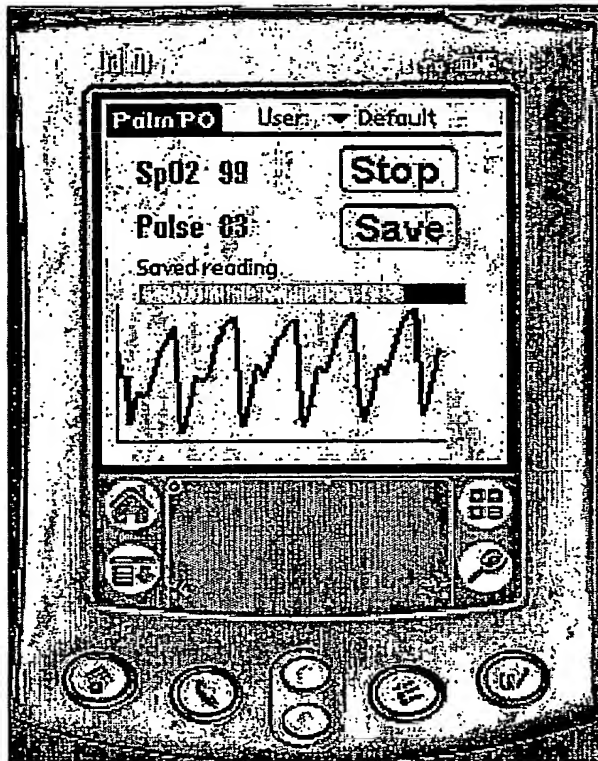


FIG. 8G

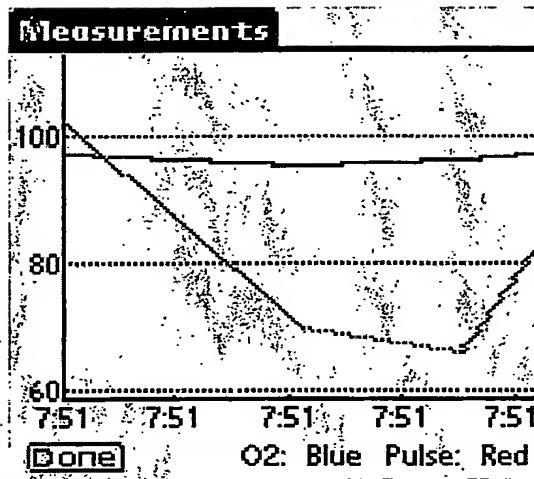


FIG. 8H

FIG. 8I is a screen titled 'Edit Patient'. It displays patient information and alarm settings. The 'Name' field is set to 'Default'. The 'Pulse Alarm' is set to 'Above 100 or Below 60'. The 'SpO2 Alarm' is set to 'Below 95'. There are 'OK' and 'Cancel' buttons at the bottom of the screen.

FIG. 8I

9/13

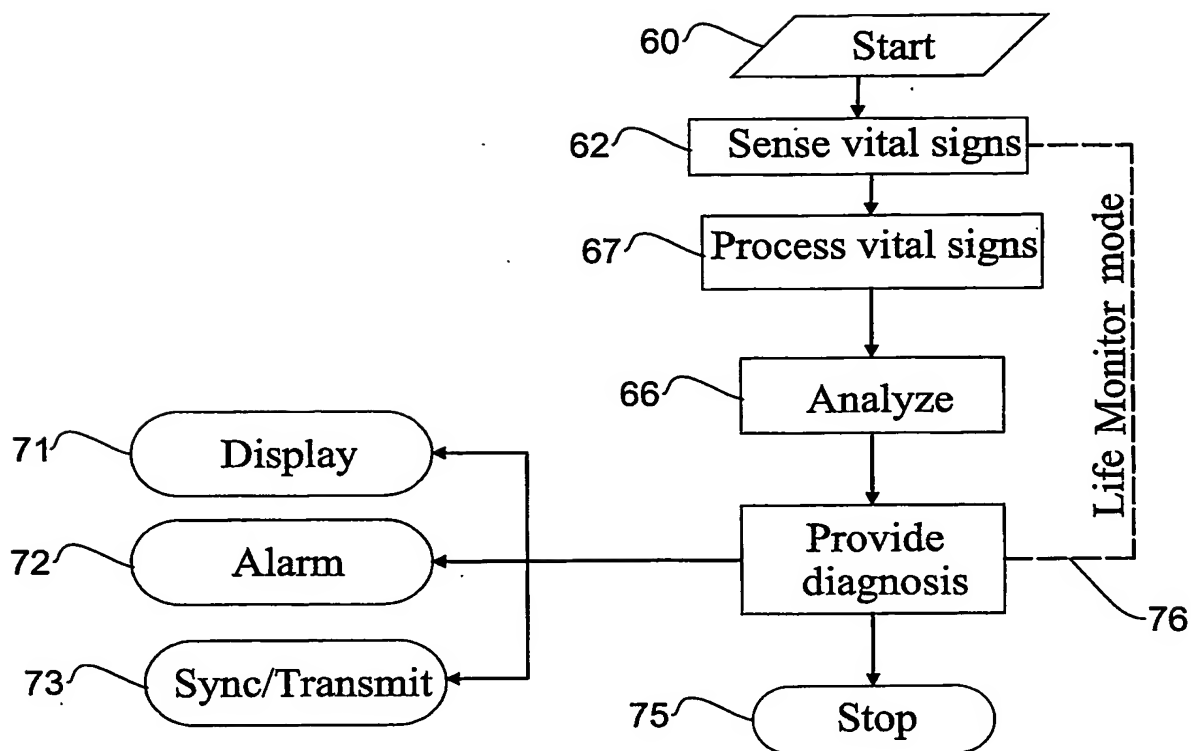


FIG. 7

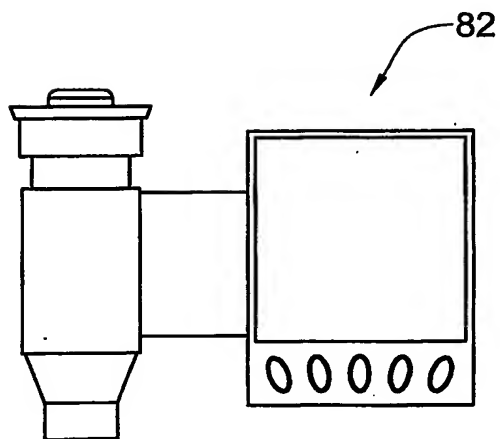


FIG. 9

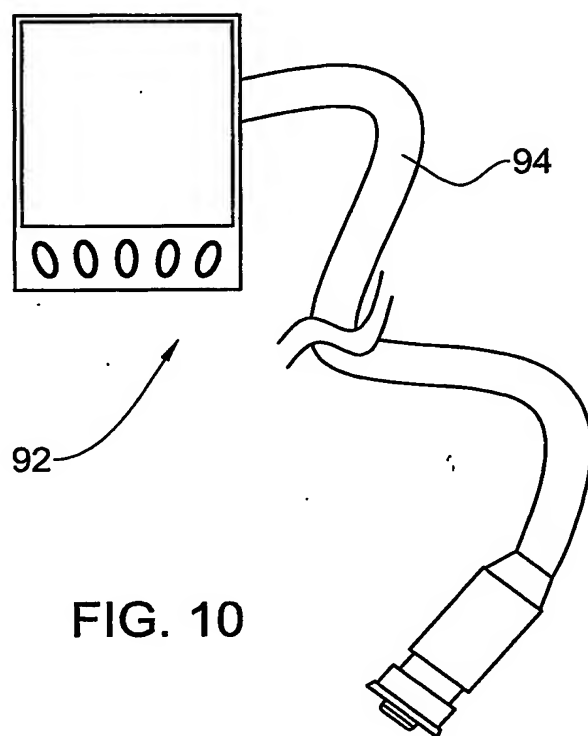


FIG. 10

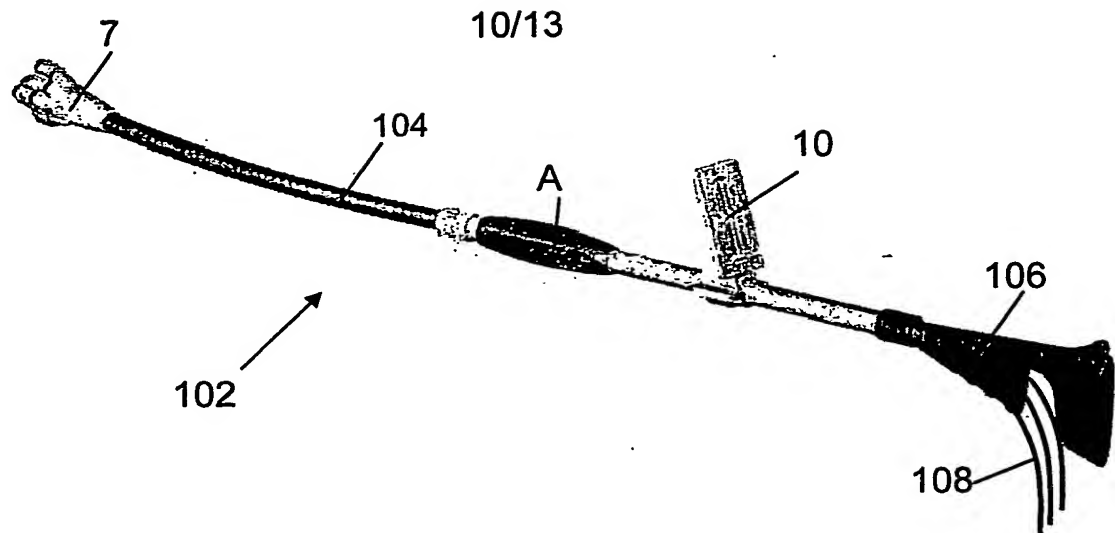


FIG. 11

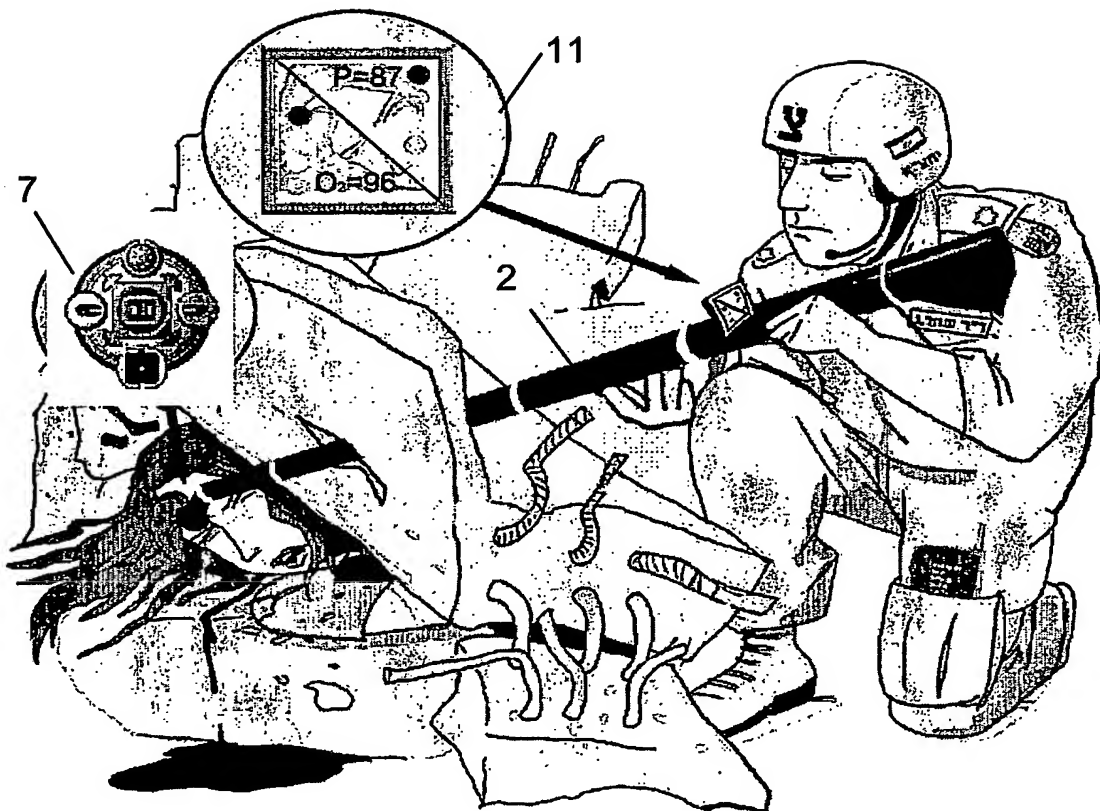


FIG. 12

11/13

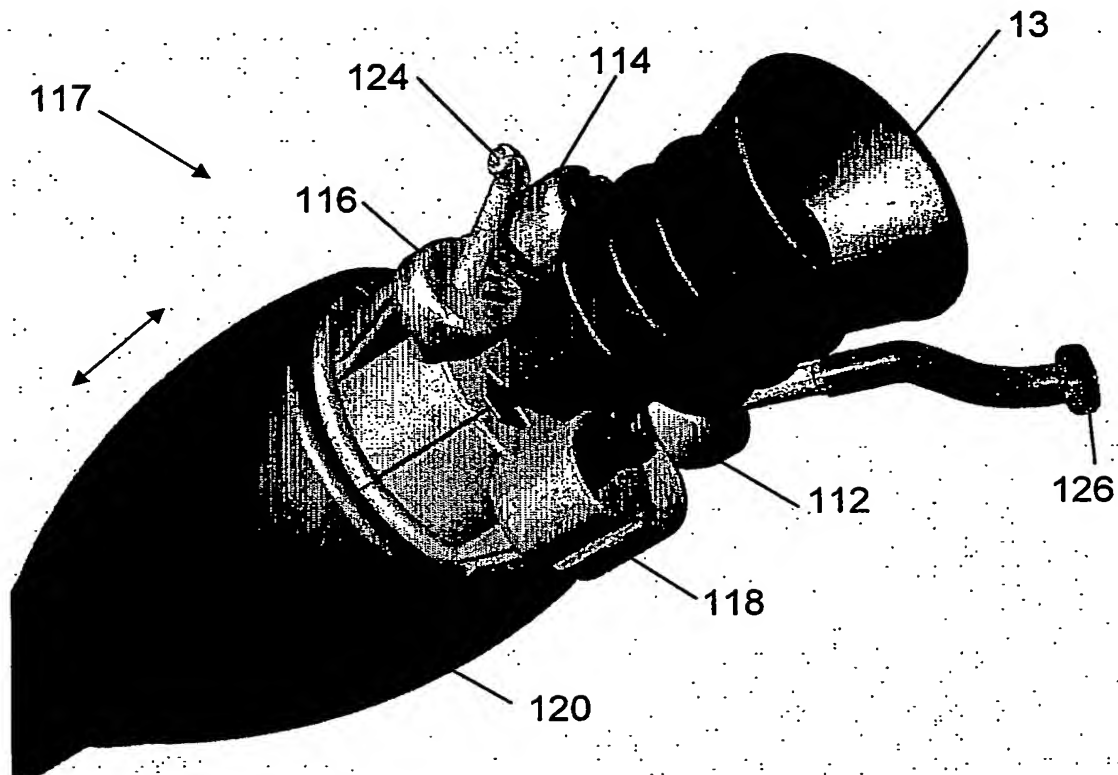


FIG. 13

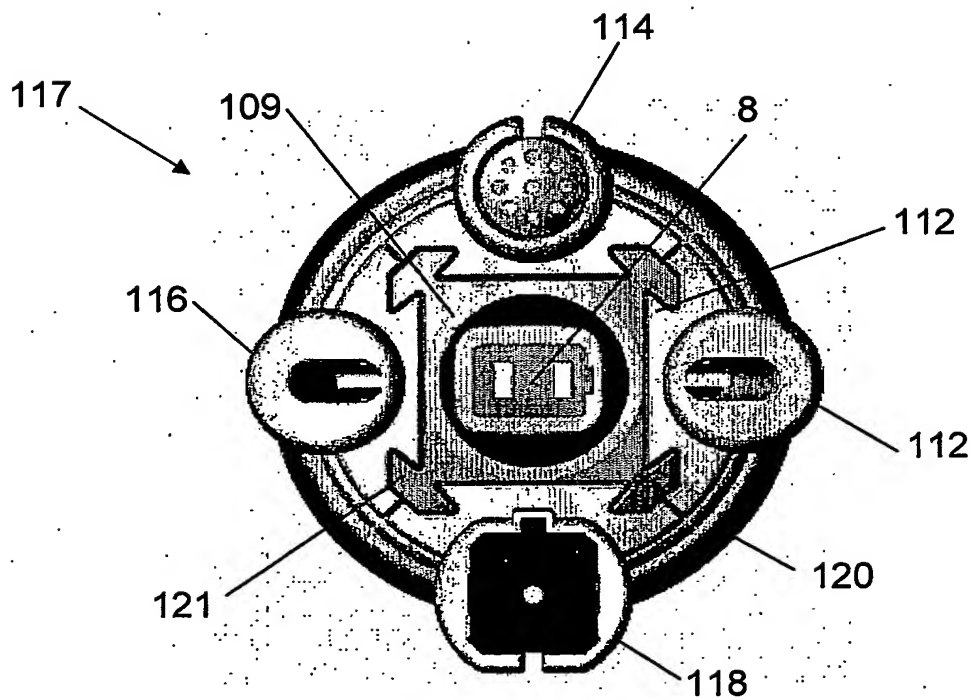


FIG. 14

12/13

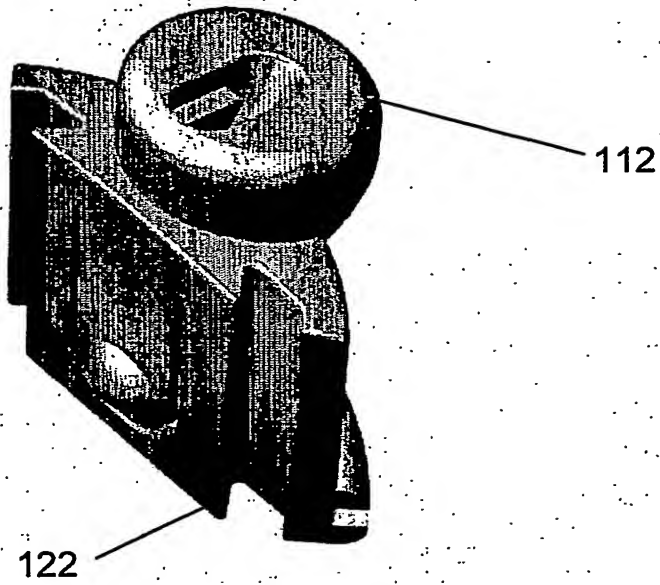


FIG. 15

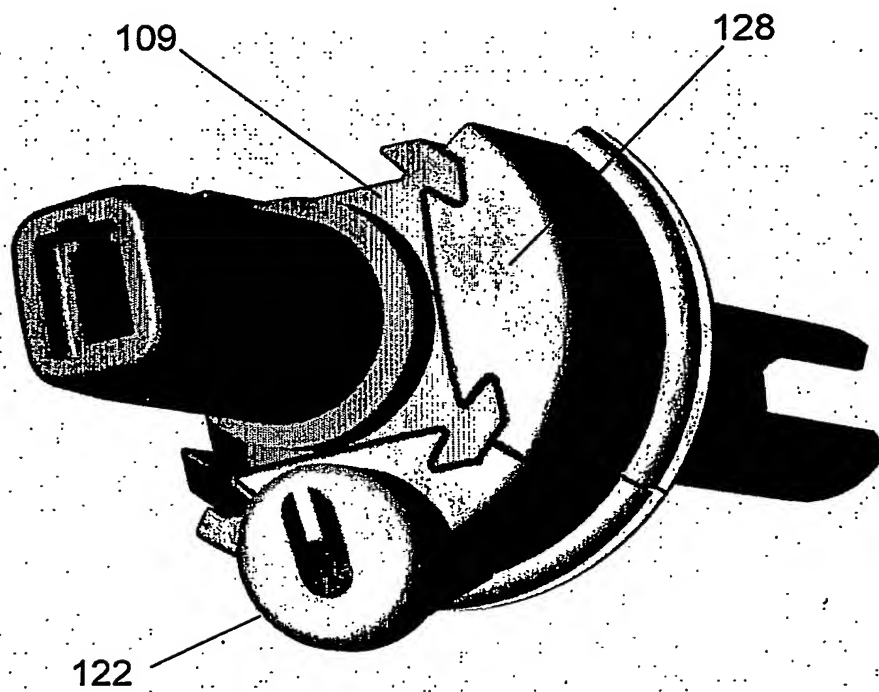


FIG. 16

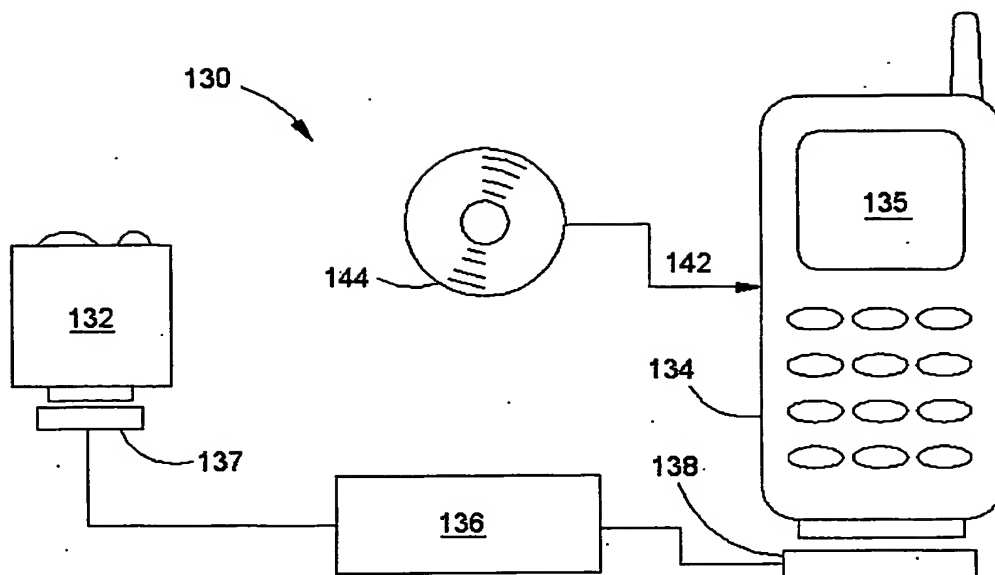


FIG. 17

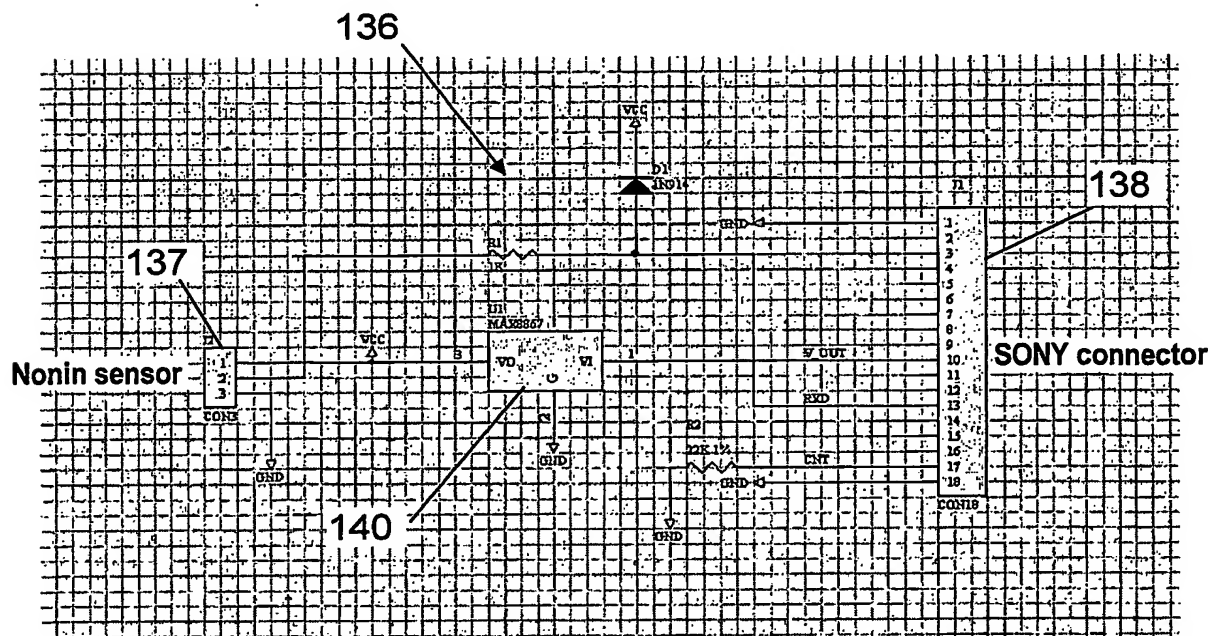


FIG. 18